

(FOR RESEARCH USE ONLY. DO NOT USE IT IN CLINICAL DIAGNOSIS!)

Cat No.: EH26040

Human CALR (Calreticulin) ELISA Kit Manual

If you have any questions or need further help during experiment, please don't hesitate to contact us through the following methods:

- ✉ Email (Order) order@enkilife.com
- ✉ Email (Techsupport) techsupport@enkilife.com
- ☎ Tel: 0086-27-87002838
- 🌐 Website: www.enkilife.com

Shelf life: Please refer to the label on the outer package.

Techsupport: In order to provide you with better service, please inform us the lot number on the label of the outer package.

Product description

This ELISA kit applies to the in vitro quantitative determination of Human CALR concentrations in serum, plasma and other biological fluids.


Key Features

- Sensitivity: 1.22ng/mL.
- Detection range: 3.12-200ng/mL.
- Specificity: It can detect Human CALR in samples without obvious cross-reaction with other analogs.
- Repeatability: The coefficient of variation within and between plates is <10%.

Test Principle

	48T: 1 vial		each experiment. Discard any unused standards after dissolution
Biotinylated Detection Ab Concentrate (100×)	96T: 120μL×1 vial	-20°C, 12 months	Unused: Please seal the concentrate and store it at -20°C, and discard the working solution
	48T: 60μL×1 vial		
HRP Conjugate Concentrate (100×)	96T: 120μL×1 vial		

Assay Procedures



them.

4. There may be a small amount of water-like substances in the wells of the newly opened ELISA plate. This is a normal phenomenon and will not affect the experimental results. Temporarily unused strips should be placed in a spare aluminum foil bag and stored according to the required storage conditions.
5. Do not reuse the diluted standard, biotinylated antibody working solution, and enzyme conjugate working solution.
6. Unused Biotinylated Detection Ab Concentrate (100×), HRP Conjugate Concentrate (100×) and other original solutions should be stored according to the required storage conditions.
7. The ELISA reader needs to be equipped with a filter that can detect a wavelength of $450\pm 10\text{nm}$, and the detection range is between 0-3.5.

assay. For short - term storage, place the sample at 2 - 8°C. Avoid using hemolyzed or hyperlipidemia samples.

3.Tissue homogenization:

3.1 For general information, hemolyzed blood may affect the results, so the tissues should be minced into small pieces and rinsed in ice-cold PBS (0.01M, pH=7.4) to remove excess blood thoroughly. Then weigh for usage.

3.2 Tissue pieces should be weighed and then homogenized in PBS (Tissue weight (g): PBS (mL) volume=1:9. It is recommended to add a protease inhibitor, such as P

4.2 Cell lysis:

Wash the cells 3 times with pre-cooled PBS. For each 1×10^6 cells, add 150-250 μL of pre-cooled PBS (If the content is very low, the volume of PBS can be reduced) to keep the cells suspended. Use an ultrasonic cell disrupter until the cells are fully lysed. (Reference settings: Use an ice bath, a 3 - 5mm probe, 150 - 300W power. Work for 1 - 2 seconds each time, with 30 - second intervals, and perform 3 - 5 cycles) Centrifuge for 10 min at $1500 \times g$. Remove the cell fragments, collect the supernatant to carry out the assay.

(1:24).Tip: The Wash Buffer Concentrate (25×) taken out of the refrigerator may have crystals, which is a normal phenomenon. You can use a 40°C water bath to slightly heat it to completely dissolve the crystals before preparing the washing solution. Use it on the same day.

4. Standard working solution:

4.1 Centrifuge the standard at 10000×g for 1 minute.

4.2 Add 1.0 mL of Reference Standard & Sample Diluent to the freeze-dried standard. After tightening the tube cap, let it stand for 10 minutes and invert it gently several times.

(100×) to 1× working solution with **Biotinylated Detection Ab Diluent**. (Biotinylated Detection Ab Concentrate (100×): Biotinylated Detection Ab Diluent= 1: 99). Prepare the working solution before use, and it should be used on the same day.

6. HRP Conjugate working solution:

Calculate the required amount before the experiment (100 µL/well), and prepare an additional 100-200µL in case of shortage. Centrifuge the **HRP Conjugate Concentrate (100×)** at 800×g for 1 min, then dilute the HRP Conjugate Concentrate (100×) to 1× working solution with **HRP Conjugate Diluent**. (HRP Conjugate Concentrate (100×): HRP Conjugate Diluent = 1: 99). Prepare the working solution before use, and it should be used on the same day.

Operation Steps

1. Add standard and sample:

Add different concentrations of **Standard working solution** to the first two columns of ELISA plate wells from top to bottom, two wells for each concentration, 100µL per well; Add 100µL of the sample to each of remaining wells. High concentration samples need to be diluted first.

During operation, solutions should be added to the bottom of the micro ELISA plate well, avoid touching the inside wall, shake gently to mix, avoid bubbles, and complete the sample addition operation within 10 minutes.

2. Cover the plate and incubate:

Cover the plate with the **Plate Sealer** provided in the kit. Incubate at 37°C for 90min.

3. Biotinylated Detection Ab working solution:

Tear off the sealer, remove and dry the liquid in the plate wells, no need to wash.

Add 100µL of **Biotinylated Detection Ab working solution** to each well. Shake gently to mix, and cover the plate with a new **Plate Sealer**. Incubate at 37°C for 60min.

4. Wash plate 1:

Manual Washing:

Aspirate or decant the liquid in the plate wells, add 350µL of **Washing solution** to each well, Soak for 1-2min, aspirate or decant the liquid in the plate wells, pat it dry against clean absorbent paper, and complete one wash. Repeat this wash step 3 times. Complete removal of liquid at each step is essential to good performance.

Microplate Washer:

350µL/well, shake the plate for 3–5 seconds.

5. Add HRP Conjugate working solution:

Add 100µL of **HRP Conjugate working solution** to each well. Gently shake to mix, cover the plate with a new **Plate Sealer**. Incubate at 37°C for 30min.

6. Wash plate 2:

Wash the plate 5 times, the steps are the same as step 4 (**Wash plate 1**).

7. Add Substrate Reagent (TMB):

Add 90µL of **Substrate Reagent (TMB)** to each well. Cover the plate with a new **Plate Sealer**. Incubate at 37°C for about 15min, Protect the plate from light.

Tips: Adjust the incubation time according to the color change, but do not exceed 30 minutes. Once the standard wells show a clear gradient, the incubation can be stopped.

8. Stop the reaction:

Add 50µL of **Stop Solution** to each well to stop the reaction.

Tip: The order of adding Stop Solution should be as consistent as possible with the order of adding Substrate Reagent (TMB).

9. Measure the OD value:

Immediately measure the OD value (optical density) of each well of the ELISA plate with a micro-plate reader set to 450nm.

📍 Calculation of results

1. Create a standard curve:

Average the duplicate readings for each standard, control, and sample and subtract the average zero standard optical density.

Create a four-parameter logistic (4-PL) curve using the curve fitting software offered by the microplate reader by plotting the mean OD value for each standard on the y-axis against the concentration on the x-axis.

2. Calculation of sample concentration:

Substitute the OD value of the sample into the standard curve to get the concentration. If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

3. Processing of high OD value samples:


If the OD of the sample surpasses the upper limit of the standard curve, the sample should be appropriately diluted and re-measured.

Technical Data

Typical Data:

The following data is for reference only. A standard curve must be run with each assay.

Concentration: ng/mL	200	100	50	25	12.5	6.25	3.13	0
OD	2.37	1.459	0.882	0.386	0.265	0.176	0.135	0.088
Corrected OD	2.282	1.371	0.794	0.298	0.177	0.088	0.047	-

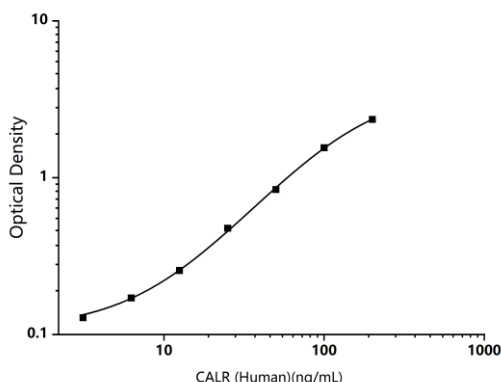

Precision:

Intra-Assay Precision (Precision within an assay): Three samples of known concentration were tested twenty times on one plate to assess intra-assay precision.

Inter-Assay Precision (Precision between assays): Three samples of known concentration were tested in twenty separate assays to assess inter-assay precision. Assays were performed by at least three technicians using two lots of components.

	Intra-assay Precision			Inter-assay Precision		
Sample	1	2	3	1	2	3
n	20	20	20	20	20	20
Mean (ng/mL)	9.56	19.21	76.98	9.58	20.12	72.53
Standard deviation	0.62	1.06	2.44	0.55	0.85	2.85
CV (%)	6.48	5.54	3.17	0.55	4.23	3.93

Recovery:

The recovery of Human CALR spiked to three different levels in samples throughout the range of the assay in various matrices was evaluated.

Sample Type	Range (%)	Average Recovery (%)
-------------	-----------	----------------------

Serum (n=5)	92-104	98
EDTA plasma (n=5)	87-100	92
Cell culture media (n=5)	95-108	100

Linearity:

To assess the linearity of the assay, samples containing and/or spiked with high concentrations of Human CALR in various matrices were diluted with the Reference Standard & Sample Diluent to produce samples with values within the dynamic range of the assay.

		Serum (n=5)	Plasma (EDTA)(n=5)	Cell culture media (n=5)
1:2	Range (%)	87-98	90-106	84-98
	Average (%)	93	97	90
1:4	Range (%)	90-102	85-97	85-97
	Average (%)	95	97	91
1:8	Range (%)	89-103	90-104	88-98
	Average (%)	95	97	91
1:16	Range (%)	83-97	90-102	81-92
	Average (%)	89	96	86

❶ Troubleshooting

If the results are not good enough, please take pictures and save the experimental data in time. Keep the used plate and remaining reagents. Then contact our technical support to solve the problem. Meanwhile, you could also refer to the following materials:

Problem	Causes	Solutions
Poor standard curve	Inaccurate pipetting	Check pipettes
	Improper standard dilution	Ensure briefly spin the vial of standard and dissolve the powder thoroughly by gentle mixing
	Wells are not completely aspirated	Completely aspirate wells in between steps
Low signal	Insufficient incubation time	Ensure sufficient incubation time

	Incorrect assay temperature	Use recommended incubation temperature
	Inadequate reagent volumes	Check pipettes and ensure correct preparation
	Improper dilution	Check dilution steps
	HRP conjugate inactive or TMB failure	Mix HRP conjugate and TMB, rapid coloring
Low value	Plate reader setting is not optimal	Verify the wavelength and filter setting on the Microplate reader(450nm)
		Open the Microplate Reader ahead to pre-heat at least 15 min
Large CV	Inaccurate pipetting	Check pipettes.
High background	Concentration of target protein is too high	Use recommended dilution factor
	Plate is insufficiently washed	Review the manual for proper wash. If using a plate washer, check that all ports are unobstructed. Ensure to use the wash buffer supplied in the Elisa kit
	Contaminated wash buffer	Prepare fresh wash buffer
Low sensitivity	Improper storage of the ELISA kit	All the reagents should be stored according to the instructions
	Stop solution is not added	Stop solution should be added to each well before measurement.

①Statement:

1. Quality and Technical Risk Tips: Limited by current conditions and scientific technology, we can't conduct comprehensive identification and analysis on all the raw material provided. So there might be some qualitative and technical risks for users using the kit.

2. Factors affecting experimental results: The experimental results are affected by many factors such as the effectiveness of the reagents, the skills of the operator and the experimental environment. To ensure the accuracy of the results, please prepare sufficient samples to be tested.

3. Reagent Usage Guide: To obtain the best experimental results, it is recommended to only use the reagents provided in this kit and operate strictly in accordance with the instructions. Avoid mixing with products from other manufacturers.

4. Operation Precautions: Improper reagent preparation or microplate reader parameter settings may lead to abnormal experimental results. Please read the instructions carefully before the experiment and adjust the instrument parameters correctly.

5. Result Reproducibility: Even the same operator may get different results in two independent experiments. To ensure the reproducibility of the results, please strictly control every step of the operation during the experiment.

6. Quality Assurance and Difference Description: Every kit has strictly passed QC test. However, results from users might be inconsistent with our data due to some variables such as transportation conditions, different lab equipment, and so on. Intra-assay variance among kits from different batches might arise from the above reasons too.

7. This kit is for research use only, do not use it in clinical diagnosis!

☐ We are always committed to providing high-quality products and thank you for your understanding and support. If you have any questions, please feel free to contact our technical support team.